

TEST REPORT



Report No. : 16-025346-01

Page of Pages : (1) / (6)



1. Client

Name : SeoJin Instech Co., Ltd

Address : 12, Sagimakgol-ro 148beon-gil, Jungwon-gu, Seongnam-si, Gyeonggi-do, 462-807, Korea

Date of Receipt : 2016. 05. 03

2. Use of Report : For Quality Control

3. Test Sample

Description : Remote Drum Level Indicator

Manufacturer : SeoJin Instech Co., Ltd

Model Name : SDG-3000

Serial Number : -

Remark : -



4. Date of Test : 2016. 05. 23. ~ 2016. 05. 24.

5. Test Standard/Method : IEC 60529: 2001

6. Testing Environment : Temperature : (20.0 ± 2.0) °C , Humidity : (66 ± 2) % R.H.

7. Test Results : Pass (IP65)

Note : 1. The test results contained apply only to the test sample(s) supplied by the client
2. This test report shall not be reproduced in full or in part without approval of the KTL in advance.

Affirmation	Tested by	Technical Manager
	Name : Chae Hui dong  (Signature)	Name : Kim Ji-hoon  (Signature)

The above test report is the accredited test result by Korea Laboratory Accreditation Scheme, which signed the ILAC-MRA.

2016. 05. 25


Korea Testing Laboratory

Accredited by KOLAS, Republic of KOREA



87, Digital-ro 26-gil, Guro-gu, Seoul, KOREA Tel.+82-2-860-1537 Fax. +82-2-860-1549



FP202-03-03



※ 위 마크는 추후 전자확인증 대조 프로그램에서 원본대조시 사용되는 2D코드입니다.

<Contents>

1. Summary of Test	3
1.1 Test Standard	3
1.2 Test Sample	3
1.3 Remark	3
2. Results	4
2.1 Dust Test Conditions	4
2.2 Dust Test Contents	4
2.3 Water Test Conditions	4
2.4 Water Test Contents	4
3. Test Figures	5
4. List of Testing Equipments	6



1. Summary of Test

1.1 Test Standard

This test was conducted in accordance with "IEC 60529: 2001".

1.2 Test Sample

- Description : Remote Drum Level Indicator
- Model Name : SDG-3000
- Dimensions : 385 mm × 260 mm × 100 mm
- Rating : 220 Vac, 50/60 Hz, 20 W



Front





Side

[Fig. 1] Test Sample

1.3 Remark

N/A




2. Results


Code Letters	IP	Conditions	Results
1st Characteristic numerals Against ingress of solid foreign objects	6	2.1 Dust Test Conditions <ul style="list-style-type: none"> Talcum powder(mesh) wire diameter : 50 μm Talcum powder(mesh) wire width : 75 μm Amount of talcum powder of the test chamber : 2 kg/m^3 2.2 Dust Test Contents <ul style="list-style-type: none"> Volume of the enclosures : About 8 000 cm^3 Reduction air pressure : -2.00 kPa (-200 mmH₂O) Flow rate : 0.20 LPM Extraction rate per hour : 1.5 volumes/h Test duration : 8 h 	Pass
2nd Characteristic numerals Against ingress of water with harmful effects	5	2.3 Water Test Conditions <ul style="list-style-type: none"> Internal diameter of the nozzle : 6.3 mm Delivery rate : 12.5 \times (1 \pm 5%) LPM Core of the substantial stream : Circle of 40 mm diameter at 2.5 m distance from the nozzle Distance from nozzle to enclosure surface : 2.8 m 2.4 Water Test Contents <ul style="list-style-type: none"> Test duration : 3 min 	Pass

※ Test Environment


- Temperature : (20.0 \pm 2.0) °C
- Humidity : (66 \pm 2) % R.H.
- Atmospheric Pressure : (101.0 \pm 2.0) kPa



3. Test Figures

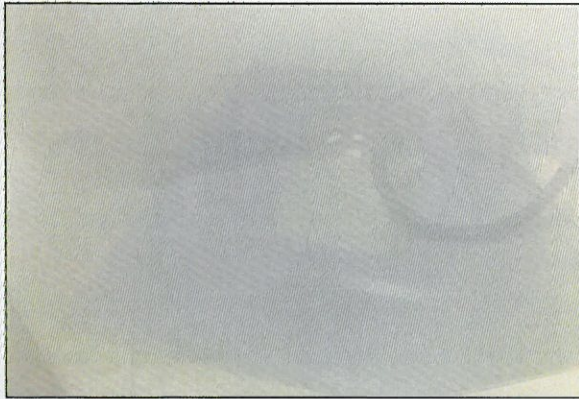


IP 6X (Dust)

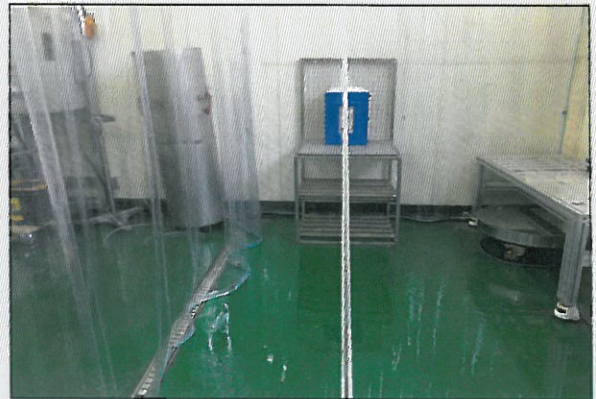

IP X5 (Water)

[Fig. 2] Test Setup



4. List of Testing Equipments

Apparatus	Manufacture	Model	Serial No.	Date of Calibration	Calibration Laboratory
Thermo-hygrometer	TESTO	Testo 622	-	2016. 05. 10	KTL
Vernia Caliper	MITUTOYO	Vernia Caliper	7003344	2015. 09. 15	KTL
Nozzle	DAEKYUNG ENGINEERING	IEC 60529	-	2016. 05. 16	KTL
Compact Dust Chamber	SCM TECHNOLOGY	PLN600-2	-	2016. 05. 10	KTL


복사본 COPY

COPY 복사본

한국산업기술시험원

- End -

FP202-02-02



※ 위 마크는 추후 전자확인증 대조 프로그램에서 원본대조시 사용되는 2D코드입니다.